Accumark Labs

CERTIFICATE OF ANALYSIS

Vigor Peptides
info@vigorpeptides.com
http://VigorPeptides.com

SAMPLE NAME: KPV + GHK-Cu + BPC-157 + TB500 (Thymosin Beta 4)
SAMPLE CODE: BGY4-V8GT
RECEIVED DATE: 05/28/2026
PUBLISHED DATE: 06/03/2026

DECLARED IDENTITY	KPV, GHK-Cu, BPC-157, TB500 (17-23 Fragment)
MATRIX TYPE:	PEPTIDE BLEND
SAMPLE NAME:	KPV + GHK-Cu + BPC-157 + TB500 (Thymosin Beta 4)
SAMPLE SIZE:	80.0 mg
Nº LOT CODE:	EST26E

87.21 mg
Total Quantity

99.75%
Total Blend Purity

Sample	Test	Specification	Result	Status
Peptide Blend	IDENTITY	KPV, GHK-Cu, BPC-157, TB500 (17-23 Fragment)	KPV, GHK-Cu, BPC-157, TB500 (17-23 Fragment)	CONFORMS
Peptide Blend	QUANTITY	MEASURE	87.21 mg	MEASURED
Peptide Blend	PURITY	> 98.0%	99.75%	CONFORMS

HPLC Chromatogram Report

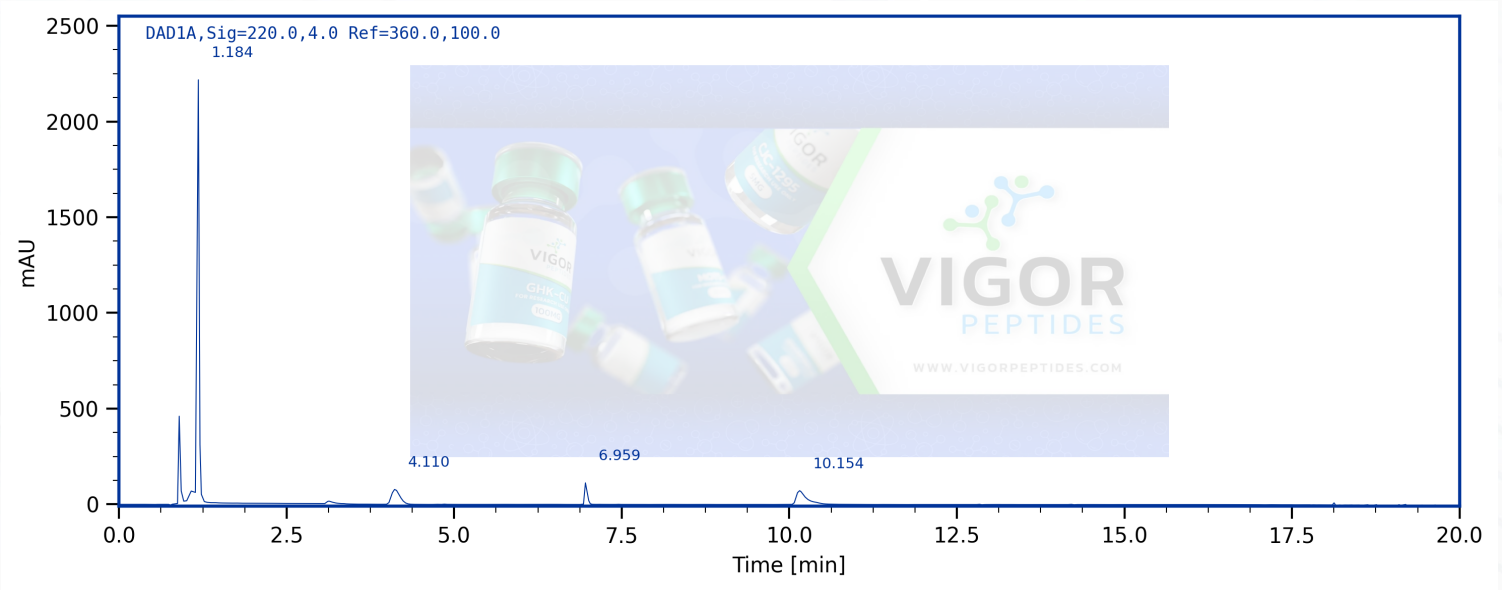

RESULTS REVIEWED BY:
Anthony Burke PhD
Lab Manager
06/03/2026

RESULTS CERTIFIED BY:
Dr. Levi Fried MD
Lab Director
06/03/2026

ACCUMARKLABS.COM
BGY4-V8GT
06/03/2026

Accumark Labs

CERTIFICATE OF ANALYSIS

Vigor Peptides
info@vigorpeptides.com
http://VigorPeptides.com

SAMPLE NAME: KPV + GHK-Cu + BPC-157 + TB500 (Thymosin Beta 4)
SAMPLE CODE: BGY4-V8GT
RECEIVED DATE: 05/28/2026
PUBLISHED DATE: 06/03/2026

Sample	Test	Specification	Result	Status
Peptide Blend	Endotoxin (LAL)	< 5.0 EU/mL	Pass	CONFORMS
Peptide Blend	Rapid Sterility Screening (PCR)	Not Detected	Pass	CONFORMS

Analyte	Test	Specification	Result	Status
KPV	IDENTITY	KPV	KPV	CONFORMS
KPV	QUANTITY	MEASURE	10.94 mg	MEASURED
KPV	PURITY	> 98.0%	99.18%	CONFORMS
GHK-Cu	IDENTITY	GHK-Cu	GHK-Cu	CONFORMS
GHK-Cu	QUANTITY	MEASURE	53.77 mg	MEASURED
GHK-Cu	PURITY	> 98.0%	99.96%	CONFORMS
BPC-157	IDENTITY	BPC-157	BPC-157	CONFORMS
BPC-157	QUANTITY	MEASURE	10.29 mg	MEASURED
BPC-157	PURITY	> 98.0%	99.28%	CONFORMS
TB500 (17-23 Fragment)	IDENTITY	TB500 (17-23 Fragment)	TB500 (17-23 Fragment)	CONFORMS
TB500 (17-23 Fragment)	QUANTITY	MEASURE	12.21 mg	MEASURED
TB500 (17-23 Fragment)	PURITY	> 98.0%	99.75%	CONFORMS

RESULTS CERTIFIED BY:

Anthony Burke PhD
Lab Manager
06/03/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
06/03/2026

ACCUMARKLABS.COM
BGY4-V8GT
06/03/2026